

Hall Effect DC Current Sensor CYCTD-S3 with Analog and Digital Outputs

The sensor CYCTD-S3 works according to Magnetic Modulation and is designed for applications to measurement and monitoring of DC current. The sensor has a galvanic isolation between the high power primary conductor and the secondary electronic circuit. The sensor has different analog and digital output signals under different power supplies. The data communication between sensor and digital equipment can be realized directly through the interface RS-485 MODBUS.

Features and Advantages	Applications
<ul style="list-style-type: none">• DC current measurement• High measuring accuracy• Analog and digital output signal (0-5V, 0-10V, RS-485 Modbus)• High isolation between primary and secondary circuits• No insertion losses• Temperature compensation	<ul style="list-style-type: none">• Photovoltaic equipment• Battery banks, such as, monitoring load current and charge current, verifying operation• Transportation, measuring traction power• Phase fired controlled heaters• Directly connect to PLC• Sense motor stalls and short circuits• Industrial instrumentation


1. Specifications

Analog Electrical Data:

Rated input current range	500mA, 750mA, 1A, 2A, 3A, 5A, 10A, 15A, 20A, 25A
Output signal	0-5VDC, 0-10V DC
Power supply	+12VDC, +15VDC, +24VDC
Measuring accuracy	1.0%
Linearity (10% - 100%), 25°C	±0.5% FS
Isolation	between input, output and power supply
Load resistance	≥2kΩ for voltage output
Isolation withstanding voltage	2.5 kV DC, 1min, leakage current 1mA
Response time	≤120ms
Frequency Bandwidth (-3dB)	DC – 8kHz
Thermal drift of offset voltage	≤600ppm/°C
Thermal Drift (-40°C to 85°C)	<2200ppm /°C
Quiescent power consumption	500mW – 1300mW (depending on power supply)

General Data:

Mounting	35mm DIN Rail
Case style and Window size	WS3 with aperture Ø20mm
Protection of Case	IP20
Operating temperature	-40°C ~ +85°C
Storage temperature	-40°C ~ +85°C
Relative humidity	5%~95% no dew
MTBF	≥ 100k hours



Digital Electrical Data:

Digital output	Current I (real value with 2 decimal places in binary code)
Output interface:	RS-485, MODBUS
Baud rate:	1200, 2400, 4800, 9600 (default), 19.2K, 38.4K, 57.6K, 115.2K bps
Refreshing period	0.5ms
Measuring accuracy	±0.5%FS
Linearity (10% - 100%), 25°C	±0.2%FS
Galvanic isolation	2500V rms for 1 min. per UL 1577
Bus protection	±15kV ESD protection on RS-485 input/output pins, open- and short circuit, fail-safe receiver inputs
Power consumption	<650mW (under power supply +12V)

2. Definition of Part number

CYCTD	-	S3	-	M	-	x	n	y
(1)		(2)		(3)		(4)	(5)	(6)

(1)	(2)	(3)	(4)	(5)	(6)
Series name	Case style	Rated input current (M=U/B+m)	Analog output voltage	Power supply	Interface
CYCTD	S3	m = 500mA, 750mA, 1A, 2A, 3A, 5A, 10A, 15A, 20A, 25A	x=3: 0-5V DC x=8: 0-10V DC	n=2: +12V DC n=3: +15V DC n=4: +24V DC	x=3: RS485, MODBUS

U: unidirectional;


B: bidirectional (please give U or B in the part number)

Example 1: CYCTD-S3-U10A-823 for DC Current Sensor with
Rated input current: 0-10A DC
Analog output voltage: 0-10V DC
Power supply: +12V DC
Interface: RS-485, MODBUS


Example 2: CYCTD-S3-B10A-823 for DC Current Sensor with
Rated input current: -10A ~ 0 ~ 10ADC
Analog output voltage: 0 ~ 5V ~ 10VDC
Power supply: +12V DC
Interface: RS-485, MODBUS

Relation between Input and Output:

Sensor CYCTD-S3-U10A-823		Sensor CYCTD-S3-B10A-823	
Input current (A)	Output voltage (V)	Input current (A)	Output voltage (V)
0	0	-10	0
2.5	2.5	-5	2.5
5	5	0	5
7.5	7.5	5	7.5
10	10	10	10




3. Case Style and Connection

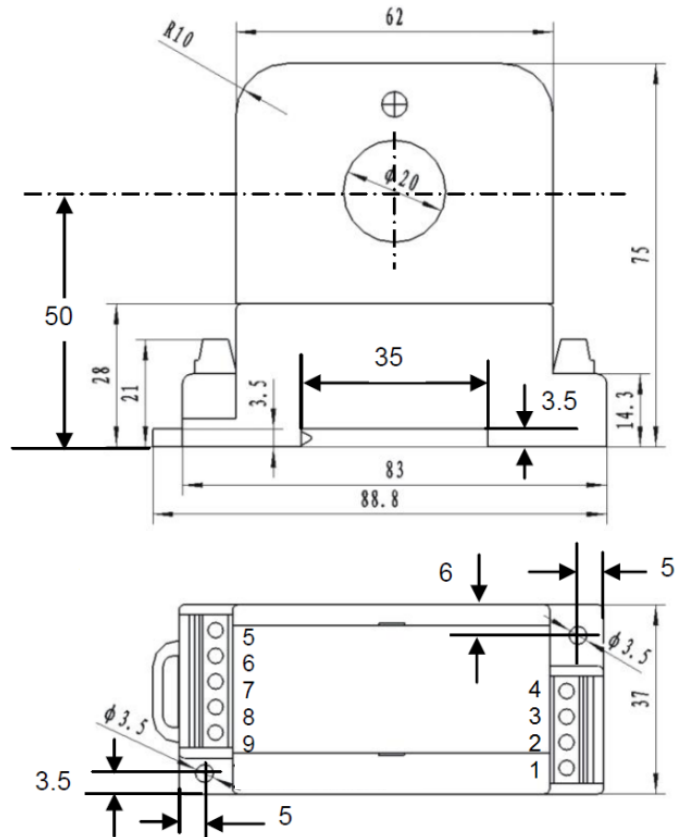


Case S3 with aperture $\varnothing 20\text{mm}$


83 x 37 x 75mm

Connection to Master Equipment with RS-485 interface

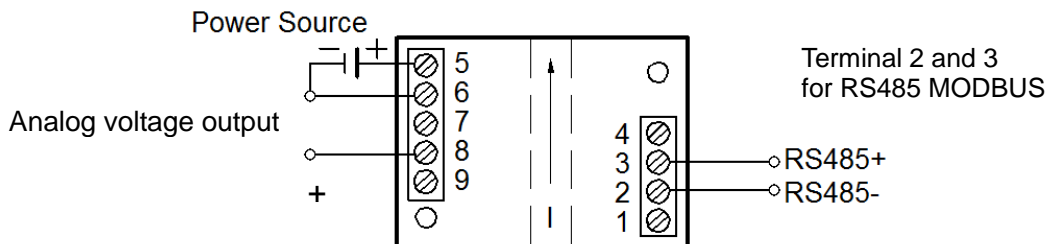

Wiring of Terminals for voltage output:

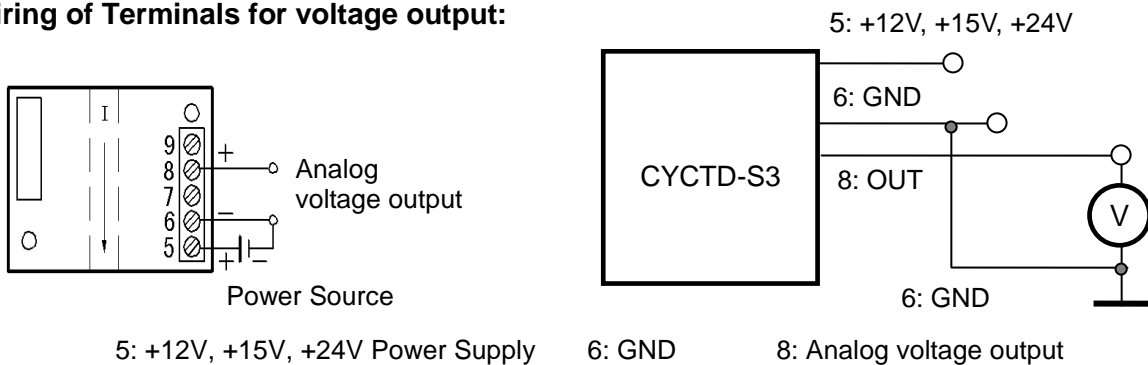



4. Communication Protocol and Order Sets

The orders of the digital Hall Effect current sensor series CYCTD are MODBUS format. Their output communication protocol is RS-485 interface protocol.

4.1 Register Address Table

Register Address	Content	Register Number	R/W	Data Range
0x0010	Reserved	1		
0x0011	Current	1	R	According to measuring range
0x0012-0x001F	Reserved	14		
0x0020	Address and baud rate	1	R/W	Address 0x01-0xF7 Baud rate 0x03-0x0A
0x0021	Device name	2	R	"CTS3"
0x0023	Serial data format	1	R/W	Parity check 0x00-0x02 Length of stop bit 0x00-0x02
0x0024	Internal output low-pass filter cutoff frequency*10	1	R/W	1-10000
0x0025-0x002F	Reserved	11		

Notice: 0x means the number is hex number, same as below.

4.2 Frame Format and Example

4.2.1 Function code 0x03 - read data from digital sensors

Request frame of master equipment

Sensor address	(0x01-0xF7	1 byte)
Function code	(0x03	1 byte)
Start register address	(2 bytes)	
Register number	(2 bytes)	
CRC	(2 bytes)	

Notice: CRC means Cyclic Redundancy Check. In this product CRC is calculated according to CRC-16 (Modbus) standard, same as below.


Examples:

(1) Read current value

Address	Function	Register Address	Register Number	CRC-L	CRC-H
0x01	0x03	0x00 0x11	0x00 0x01	0xD4	0x0F

(2) Read device name and settings

Address	Function	Register Address	Register Number	CRC-L	CRC-H
0x01	0x03	0x00 0x20	0x00 0x05	0x84	0x03



4.2.2 Function code 0x10 --- write data to digital sensors

Request frame of master equipment

Sensor address	(0x01-0xF7	1 byte)
Function code	(0x10	1 byte)
Start register address	(2 bytes)	
Register number	(2 bytes)	
Data byte length	(2*register number	1 byte)
Data write to register	(2*register number bytes)	
CRC	(2 bytes)	

Examples:

(1) Change address and baud rate

Address from 01 (default) to 02, baud rate from 9600 (default) to 19.2K.

Address	Function	Register Address		Register Number		Data Number	Data		CRC-L	CRC-H
0x01	0x10	0x00	0x20	0x00	0x01	0x02	0x02	0x07	0xE1	0x92

Explanation:

Data 0x0207 is written into register 0x0020. The high byte 0x02 means the sensor address on the RS485 bus. The low byte 0x07 means the baud rate of communication.

(2) Change serial data format

Parity check from none (default) to even, length of stop bit from 1 bit (default) to 2 bits.

Address	Function	Register Address		Register Number		Data Number	Data		CRC-L	CRC-H
0x01	0x10	0x00	0x23	0x00	0x01	0x02	0x02	0x02	0x21	0xA2

Explanation:

Data 0x0202 is written into register 0x0023. The high byte 0x02 means the parity check. The low byte 0x02 means the length of stop bit.


(3) Change cutoff frequency of internal output low-pass filter

From no low-pass filter (default) to cutoff frequency 65.5Hz.

Address	Function	Register Address		Register Number		Data Number	Data		CRC-L	CRC-H
0x01	0x10	0x00	0x24	0x00	0x01	0x02	0x02	0x8F	0xE0	0x70

Explanation:

This current sensor has a first order digital low-pass filter for output, which keeps the output result with higher stability when cutoff frequency is low. But a lower cutoff frequency also causes slower response. User can turn off this low-pass filter or adjust the cutoff frequency by setting this register.



Data 0x028F is written into register 0x0024. 0x028F=655, which corresponds cutoff frequency 65.5Hz.

Answer frame of digital sensors

Sensor address	(0x01-0xF7	1 byte)
Function code	(0x10	1 byte)
Start register address	(2 bytes)	
Register number	(2 bytes)	
CRC	(2 bytes)	

Examples:

(1) Received correct answer of changing address and baud rate

Address	Function	Register Address		Register Number		CRC-L	CRC-H
0x01	0x10	0x00	0x20	0x00	0x01	0x00	0x03

(2) Received correct answer of changing serial data format

Address	Function	Register Address		Register Number		CRC-L	CRC-H
0x01	0x10	0x00	0x23	0x00	0x01	0xF0	0x03

(3) Received correct answer of changing cutoff frequency

Address	Function	Register Address		Register Number		CRC-L	CRC-H
0x01	0x10	0x00	0x24	0x00	0x01	0x41	0xC2

4.2.3 Error frame from digital sensors


Error frame of digital sensors

Sensor address	(0x01-0xF7	1 byte)
Function code	(0x80 function code	1 byte)
Error Code	(0x01-0x04	1 byte)
CRC	(2 bytes)	

The symbol “|” means logic “OR”

Error code

- 0x01: illegal function
- 0x02: illegal register address
- 0x03: illegal data value or register number
- 0x04: sensor failures (read or write error)



Examples:

(1) Wrong function code has been send

For example, the function code 0x04 has been sent in a sending frame. Received error answer is

Address	Function	Error Code	CRC-L	CRC-H
0x01	0x84	0x01	0x82	0xC0

(2) Wrong register address has been send

The sending frame is for reading the current value as showed in paragraph 4.2.1, but the register address is 0x0001. Received error answer is

Address	Function	Error Code	CRC-L	CRC-H
0x01	0x83	0x02	0xC0	0xF1

(3) Wrong register number has been send

The sending frame is for reading device name and settings as showed in paragraph 4.2.1, but the register number is 0x0010. In this situation, the last register address that should be written is 0x0030, which is beyond the valid address range 0x0010 to 0x002F. Received error answer is

Address	Function	Error Code	CRC-L	CRC-H
0x01	0x83	0x02	0xC0	0xF1

(4) Register number must be greater than 0

The sending frame is for reading the current value as showed in paragraph 4.2.1, but the register number is 0x0000. Received error answer is

Address	Function	Error Code	CRC-L	CRC-H
0x01	0x83	0x03	0x01	0x31

(5) Wrong data number has been send


The sending frame is for changing cutoff frequency as showed in paragraph 4.2.2, but the data number is 0x03, which doesn't match register number*2. Received error answer is

Address	Function	Error Code	CRC-L	CRC-H
0x01	0x90	0x03	0x0C	0x01

(6) Data written is beyond valid data range

The sending frame is for changing device address and baud rate as showed in paragraph 4.2.2, but the data is 0xF807, which is beyond the valid device address range 0x01-0xF7. Received error answer is

Address	Function	Error Code	CRC-L	CRC-H
0x01	0x90	0x03	0x0C	0x01



(7) The case (0x04: Sensor failures) should not occur in this sensor

Notes:

1. If digital sensor address or CRC is wrong, no answer frame or error frame will be back from sensor.
2. Low byte of CRC is transmitted first. By register address, register number and data, high byte is transmitted first.
3. Register word length is 16 bits (2 bytes).
4. Every valid request frame has a corresponding answer. The master equipment should send the next request after the answer has been received. The maximum waiting time for data reading equals to the data refreshing period. And the waiting time for configuration changing is up to 25ms.

Application Notes:

1. Connect the terminals of power source, output respectively and correctly, never make wrong connection.
2. Two potentiometers can be adjusted, only if necessary, by turning slowly to the required accuracy with a small screw driver.
3. The best accuracy can be achieved when the window is fully filled with bus-bar (current carrying conductor).
4. The in-phase output can be obtained when the direction of current of current carrying conductor is the same as the direction of arrow marked on the transducer case.