

Open Loop Hall AC/DC Current Sensor CYHCS-E

This Hall Effect current sensor is based on open loop principle and designed with a high galvanic isolation between primary conductor and secondary circuit. It can be used for measurement of DC and AC current, pulse currents etc. The output of the transducer reflects the real wave of the current carrying conductor.

Product Characteristics	
 Excellent accuracy Very good linearity Light in weight Less power consumption Window structure Electrically isolating the output of the transducer from the current carrying conductor No insertion loss Current overload capability 	

Electrical Data

Primary Nominal Current <i>I</i> _r (A)	Measuring Range (A)	Output voltage (analog) (V)	Aperture Diameter (mm)	Part number
/	Range (A)			
25	± 75	4 +1.0%	Ø20.5	CYHCS-E25A-C
50	± 150			CYHCS-E50A-C
100	± 300			CYHCS-E100A-C
150	± 450			CYHCS-E150A-C
200	± 600	4 +1.0%	020.5	CYHCS-E200A-C
300	± 900			CYHCS-E300A-C
400	±1000			CYHCS-E400A-C
500	±1000			CYHCS-E500A-C

(Connector: Molex connector C=M; Phoenix Connector: C=P)

Supply Voltage	V_{cc} = ±15V ± 5%,
Current Consumption	<i>l_c</i> < 25mA
Galvanic isolation, 50/60Hz, 1min:	2.5kV
Isolation resistance @ 500 VDC	> 500 MΩ

Accuracy and Dynamic performance data

Electric Offset Voltage, T_A =25°C, V_{oe} Magnetic Offset Voltage ($I_r \rightarrow 0$) V_{om} Thermal Drift of Offset Voltage, V_{ot} Thermal Drift (-10°C to 50°C),T.C.Frequency bandwidth (- 3 dB):DC-4	<1.0% FS <±25mV <±20mV <±0.5mV/°C . < ±0.1% /°C 50kHz
Response Time at 90% of I_P (f=1k Hz) $t_r < 3$	


Version 2 Released in May 2016 Dr.-Ing. habil. Jigou Liu




General Data

Ambient Operating Temperature, Ambient Storage Temperature,

PIN Definition and Dimensions

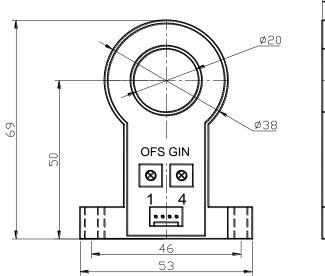






 $T_A = -25^{\circ}\text{C} \sim +85^{\circ}\text{C}$

 $T_{\rm S} = -40^{\circ} \rm C \sim +100^{\circ} \rm C$

1: V+ 2: V-3: Output 4: Ground

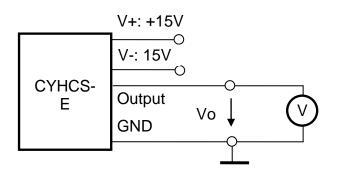



Notes:

- 1. Connect the terminals of power source, output respectively and correctly, never make wrong connection.
- 2. Two potentiometers can be adjusted, only if necessary, by turning slowly to the required accuracy with a small screwdriver.
- 3. The best accuracy can be achieved when the window is fully filled with bus-bar (current carrying conductor).
- 4. The in-phase output can be obtained when the direction of current of current carrying conductor is the same as the direction of arrow marked on the transducer